User Manual

SmartMat™

Part of the Podimetrics Remote Temperature Monitoring System™

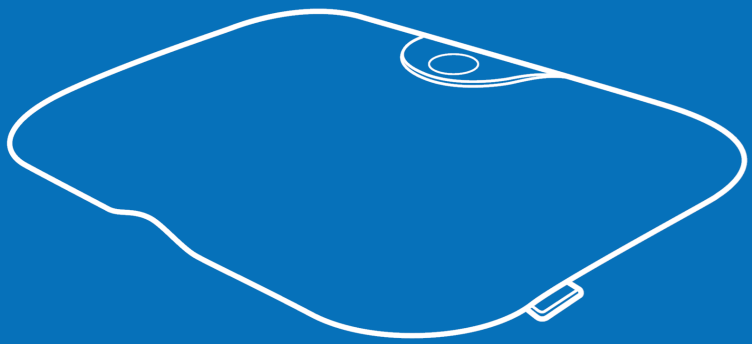

Built on proven thermometry science, the Podimetrics SmartMat™ records high resolution daily thermal scans of your feet and transmits them for evaluation by your healthcare provider.

podimetrics

ASSISTANCE INFORMATION

For technical help, please call Podimetrics, Inc.

Phone: 1-888-498-6489

Email: info@podimetrics.com

Mail: Podimetrics, Inc.
100 Dover Street
Somerville, MA 02144

Complaints related to device functionality, performance, or service can be submitted by phone or email.

ABOUT THE PODIMETRICS SMARTMAT ™

The Podimetrics SmartMat™ includes sensitive electronics to measure the temperature over the soles of the feet and transmit that data wirelessly to a remote server for evaluation. The flexible temperature sensors are positioned directly under the cover and on top of a layer of foam that compresses when you stand on it. Each thermal scan that is taken with the SmartMat is transmitted wirelessly to a server where it can be reviewed by your healthcare provider for signs of inflammation on your feet.

TABLE OF CONTENTS

4 Indications & contraindications
5 Benefits & risks
6 What is in the box
7 Description of parts
8 Setup instructions and reminder light
10 Usage instructions
12 Data transmission, monitoring notes and cleaning
13 Battery charging
14 Troubleshooting
15 What to do with your SmartMat & safety symbols
16 Guidance and Manufacturer's Declaration
19 Recommended separation distances
20 Technical information
21 Terms of Use and Privacy Policy

TABLA DE CONTENIDOS

45 Indicaciones y contraindicaciones
46 Beneficios y riesgos
48 Qué incluye la caja
49 Descripción de las piezas
50 Instrucciones de configuración y luz de recordatorio
52 Instrucciones de uso
54 Transmisión de datos y notas de monitoreo y limpieza
55 Cargando la batería
56 Solución de problemas
57 Información técnica

INDICATIONS FOR USE

The Podimetrics Remote Temperature Monitoring System™ (RTM System™) is intended to be used by a patient in conjunction with a healthcare professional or caretaker for periodic evaluation of the temperature over the soles of the feet for signs of inflammation.

It will provide information indicating when the patient and healthcare provider should communicate for further evaluation and treatment regarding any persistent localized inflammation observed on the feet via the electronic sensing system and remote visualization of its data.

The Podimetrics RTM System™ is intended to be used under the direction of a healthcare professional as an adjunct to, and not in replacement of, self-examination and periodic foot care and examination conducted by a healthcare professional and does not diagnose any specific disease state.

It is for prescription use only.

CONTRAINDICATIONS

Patients with an active ulcer or other lesions that have broken the skin on the soles of the feet should not use the Podimetrics SmartMat with the wounded foot. Patients may continue using the Podimetrics SmartMat to monitor an unwounded foot.

ESSENTIAL PERFORMANCE

The essential performance of the SmartMat™ is to take a complete scan and transmit the temperature data to a remote server.

BENEFITS AND RISKS

Benefits: It can be difficult for patients at risk for inflammatory foot diseases to evaluate the soles of their feet for signs of inflammation associated with an injury. The temperature data transmitted wirelessly by the Podimetrics SmartMat™ may be used by you and your doctor to identify signs of inflammation to your feet. With this information, your doctor may choose to initiate a physical examination and actions to avoid complications like foot ulcers, infection, gangrene, and amputation.

Risks: The Podimetrics SmartMat™ does not cause any pain or discomfort to use. The top layer has been tested for skin biocompatibility. If damaged or used improperly, inaccurate temperature readings may be taken which could affect the clinician's evaluation of inflammation.

⚠ WARNINGS

- **Do not** use the SmartMat without being trained by a healthcare professional or qualified trainer.
- **Do not** use the SmartMat if it appears damaged or contaminated.
- **Do not** use the SmartMat for more than one person because it may lead to cross-contamination or patient data mix-up.
- If any **irritation**, **redness**, or **rash** develops on the bottom of your feet, **discontinue use** and contact your healthcare provider immediately.
- If you observe any changes in SmartMat behavior or performance or any damage due to shipping or use, discontinue use and contact Podimetrics for instruction.
- **Do not** open or modify this equipment in an attempt to correct a problem. There are no user serviceable parts inside.

PRECAUTIONS

Do not place other objects or coverings on the SmartMat when it is being used. The mat's measurements may not be accurate if used with an external covering.

WHAT IS IN THE BOX

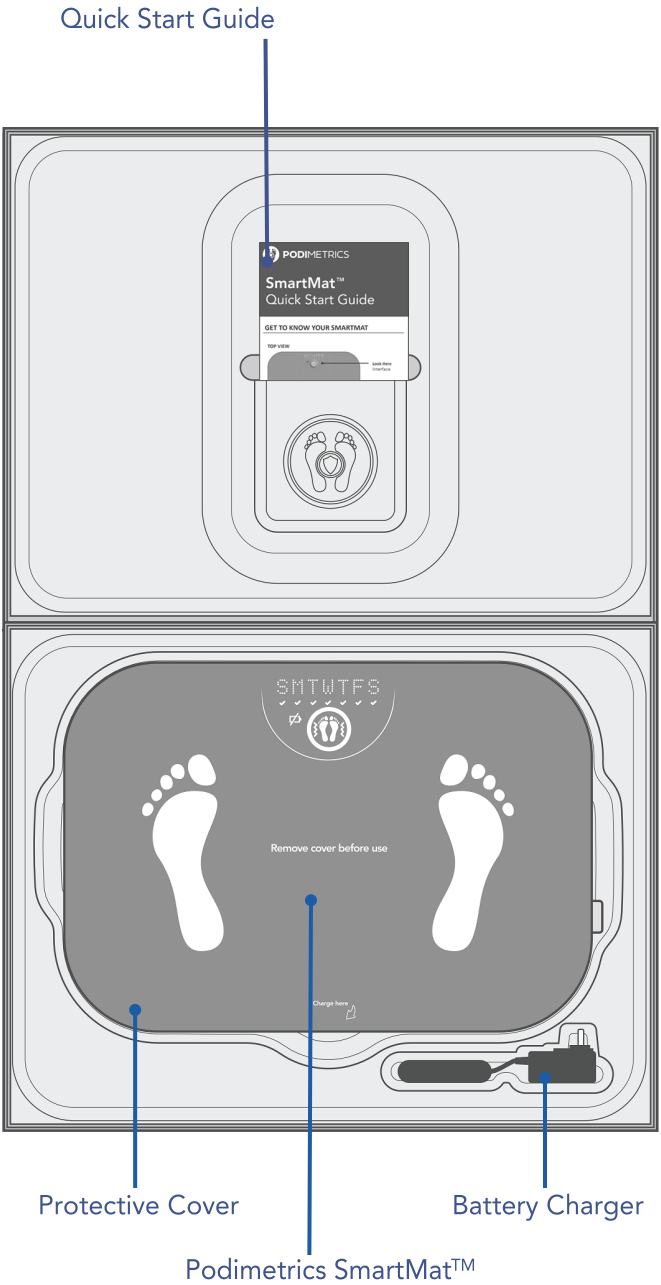

DESCRIPTION OF PARTS

TOP

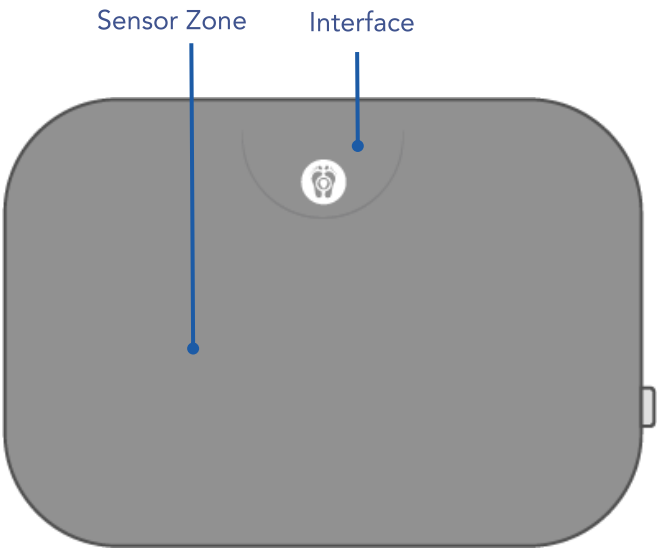

SIDE



BOTTOM

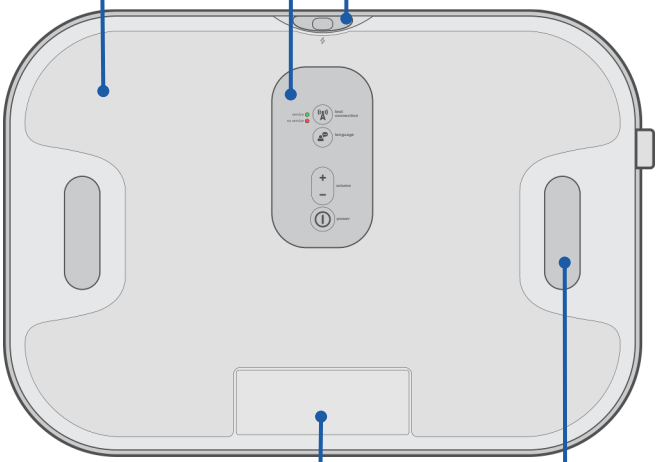

SETUP INSTRUCTIONS

1. Remove the SmartMat from the box and remove the clear protective cover: With both hands take the SmartMat out of the box and place it upside down on a table with the buttons facing up. Remove the clear plastic covering. Don't use the SmartMat if it appears damaged or contaminated.

> **NOTE: Keep the box** for storing the charger and instructions, and for shipping the SmartMat back to Podimetrics after use.

2. Turn on the mat: Press the power button. When you hear the startup chime, the SmartMat is ready to use. **Note: Keep the SmartMat on at all times** so it can send your data.

3. Set the volume: There are four (4) volume settings, Off, Low, Medium, and High. Press the volume up (+) or volume down (-) button until the audible tone is your preferred level.

4. Set the language: Press the language button to change the language of the messages. The last language you hear will be saved for future use. The default is English.

5. Check cellular service: The SmartMat automatically connects to a cellular network, just like a cellphone. To ensure the SmartMat can send your data, check the cellular service by pressing the "test connection" button and wait for the light to land on red or green. If "no service" (red light) is displayed, move the SmartMat to another location and try again.

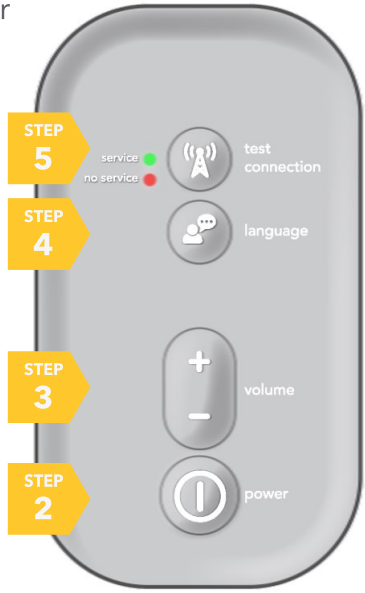

BUTTON PAD
(ON BOTTOM OF SMARTMAT)

CELLULAR SERVICE CHECK
(ON BUTTON PAD)

6. **Position the SmartMat for use:** Set the SmartMat on a flat floor where you won't trip on it and where you can comfortably stand for at least 20 seconds. The soft gray side should be facing up.

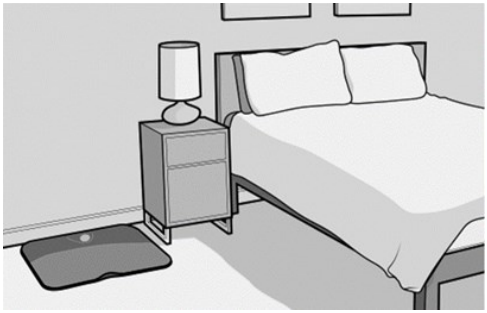

RECOMMENDED PLACEMENT

⚠ CAUTION:

- **Do not** place the SmartMat in a walkway like a hall or doorway where you might trip on it.
- **Do not** place the SmartMat in a location where it is likely to get wet, such as by a shower.
- **Do not** place the SmartMat in direct sunlight or next to heat sources like vents or space heaters.
- Place the SmartMat in a location that **minimizes the risk of tampering** by children or pets.
- Place the SmartMat in a position where you can easily **unplug it before use**.

DAILY REMINDER LIGHT

Each day, the blue reminder light will blink if you haven't taken a scan that day by 9:00 AM. You can always take a scan before the reminder light turns on.

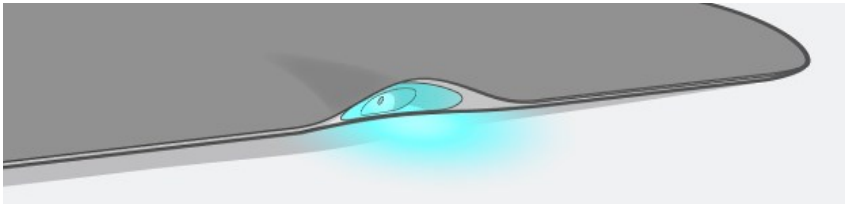

USAGE INSTRUCTIONS

NOTE: For best results, follow this process every morning.

1. Perform daily foot exam:

Continue to perform your daily foot inspection, as instructed by your healthcare provider, examining your feet for signs of developing ulcers or open wounds.

WARNING: If you notice broken skin or a developing ulcer, stop using the SmartMat and contact your healthcare provider immediately.

2. Check the mat:

Before use, inspect the SmartMat for wetness, damage, or discoloration. Make sure the SmartMat is dry before using it. If it is damaged, do not use the SmartMat and contact Podimetrics for a replacement. If it is soiled or discolored, try to clean off any residue. If the discoloration cannot be removed, contact Podimetrics to see if a replacement is necessary.

3. Stand on the mat, barefoot:

To start a scan, stand on the soft gray side of the SmartMat with both bare feet completely on the mat and spread a few inches apart. The display will say "STAY STILL". Once you are standing still, the scan will automatically start.

CAUTION: Do not use with water or lotion on your feet.

If your doctor recommends that you continue using the SmartMat while you have a bandaged wound, only step on the SmartMat with the unbandaged foot. You can place your unbandaged foot anywhere on the SmartMat when taking a scan. Always follow your doctor's instructions regarding footwear.

NOTE: Although use while standing is preferred, the SmartMat can also be used while sitting as long as enough pressure is applied to complete a scan. Do not use the SmartMat in a way that you feel may increase your risk of falling or tripping. Discuss with your doctor whether using the SmartMat while standing or sitting is most appropriate for you.

4. Complete the scan:

Keep your feet still for 20 seconds while the scan completes. The progress circle will fill up completely and turn white when the scan is done. "SCAN SAVED" will appear and the SmartMat will chime again. You can now get off the SmartMat.

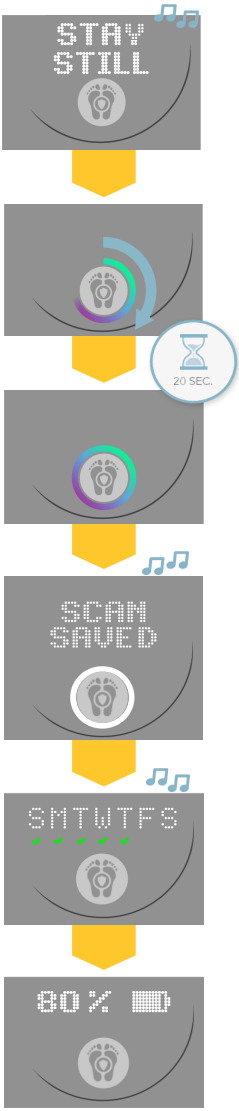

NOTE: If you move your feet during the scan, the yellow stability icon will light up and an error chime will sound, indicating the scan has been interrupted. Press down firmly with your feet and stay still for the scan to restart.

5. Check weekly scans and battery:

The SmartMat will display your weekly calendar of scans and confirm the scan for today. A green checkmark ✔ means a scan was taken for that given day. The battery level percentage is displayed on the screen. Your scan will be transmitted automatically and the SmartMat will go to sleep. Keep the power on so that your scan can be transmitted.

NOTE: You can check your recent scans and the battery level by tapping on the top surface of the mat.

NOTE: **Don't leave the SmartMat plugged in.** The SmartMat cannot take a scan with a low battery or when plugged in.

DATA TRANSMISSION & MONITORING

Data transmits automatically: If you have placed the SmartMat in a location with good cellular signal (see page 8 for instructions how to check cellular signal strength) the SmartMat will automatically transmit the data to Podimetrics through the cellular network. Cellular coverage may not be available in all regions. Contact Podimetrics if you have difficulty finding a location with good signal. The data will not be transmitted outside of the United States. The SmartMat will save at least 20 scans in memory if outside of cell signal, and it will retry transmission daily.

Podimetrics Monitoring: If Podimetrics hasn't received a scan from your SmartMat in a while, you may receive a call to make sure everything is okay with you and your mat.

Scan Review: Your healthcare provider can review the data from your SmartMat periodically for signs of inflammation. The reports they receive display thermal images of your feet and allow your healthcare provider to analyze areas of elevated temperature for each scan that is transmitted. Consult your doctor for information on thermogram evaluation.

CLEANING

Cleaning: Once per month or as needed, wipe the top surface of the SmartMat with lukewarm water and a clean cloth to remove any dirt or residue that may build up and affect the sensor reading or make it slippery. Let the SmartMat completely air dry before use. If it is difficult for you to clean while the SmartMat is on the floor, you can place it on a table.

> ⚠ **CAUTION:** Do not clean the SmartMat with soap as it may leave a slippery residue. Do not immerse the SmartMat in water.

BATTERY CHARGING

Battery charging: The battery percentage will decrease in 10% steps. The low battery light will turn on when the battery is too low to take a scan. To charge, place the SmartMat upside down on a table or counter nearby an electrical outlet. Plug in the charger to a standard wall outlet and insert the round end into the charger port. Charging an empty battery takes about four hours. While the SmartMat is plugged in, a scan cannot be taken.

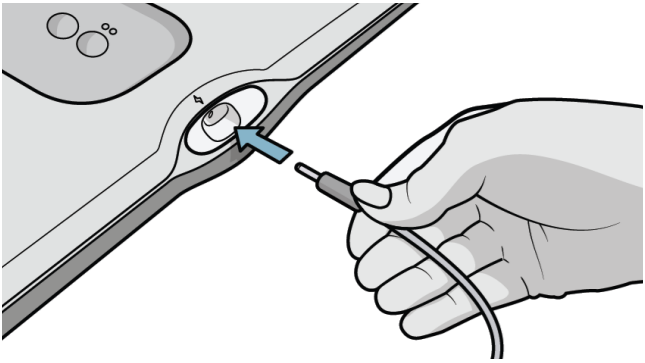

CHARGER LOCATION
(ON SIDE OF SMARTMAT)



CHARGING
(BLINKING YELLOW)

CHARGING COMPLETE
(SOLID GREEN)

NOTE: **Unplug the SmartMat before taking a scan again.** If you stand on the SmartMat while it is plugged in, an error chime will sound and "UNPLUG" will be displayed on screen.

CAUTION:

- Use only the supplied charging cable for charging. Using other cables may damage the internal electronics.
- Keep the charging cable off the floor and away from walkways to prevent creating a trip hazard.
- Keep the charging cable out of the reach of children. The charging cable may be a strangulation risk.
- Your charger may not work in other countries.

TROUBLESHOOTING

If the instructions in this table do not resolve the issue or if you experience any malfunction or injury, please call Podimetrics technical support at 1-888-498-6489.

Problem	Meaning	Action
"Low battery" light turns on.	The battery is low.	Plug in the charging cable to charge the SmartMat battery.
"No service" light turns on.	The SmartMat does not have enough cellular signal in its location.	Move the SmartMat to an area with better cellular coverage such as closer to a window or upstairs.
"Stability error" light turns on.	Your feet may have moved during the scan.	Make sure both feet are fully inside the sensing zone and stand still until the full scan is completed.
The SmartMat does not start scanning when you stand on it.	The SmartMat may be off - or - The battery may be empty	If there are no lights on, try pressing the volume UP button. If the SmartMat doesn't make a sound, press the power button to turn the SmartMat on. If the SmartMat still doesn't turn on, you may need to charge the battery.
The SmartMat does not make any sounds.	The volume may not be turned on.	Turn on the volume by pressing the volume UP (+) button on the bottom of the mat.

WHAT TO DO WITH YOUR MAT

Traveling:
Feel free to take your SmartMat with you in its box and use it at your destination. Especially when flying, turn the SmartMat off while in transit. If you don't plan to bring the SmartMat with you, call Podimetrics to inform them that you won't be using it. The SmartMat is not designed for use outside the United States.

Storage:
Store the SmartMat powered off in its shipping box in a cool, dry place out of direct sunlight. The materials may degrade over time if exposed to sunlight or high temperatures.

Return:
Contact Podimetrics for instructions for returning the used mat. Do not dispose of the SmartMat in a municipal trash facility as the electronics may be damaging to the environment.

SAFETY SYMBOLS

Do not use the product if the packaging is damaged.

Read the operating instructions carefully.

IP 21

This product is rated IP21. It is protected against inserted fingers and dripping water.

The SmartMat is a Type B applied part and is not electrically conductive with the body.

This product contains electronics. Do not dispose of in municipal waste facilities.

Rx only

This product is for prescription use only.

Device uses RF transmitter that produces non-ionizing radiation

Electromagnetic Immunity:

The Podimetrics SmartMat is intended for use in the electromagnetic environment specified below. The customer or the user of the Podimetrics SmartMat should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Conducted RF IEC 61000-4-6 Radiated HF interference quantities according to IEC 61000-4-3	3 Vrms 150 kHz to 80 MHz 3 V/m 80 MHz to 2.5 GHz	3 Vrms 3 V/m	Portable and mobile RF communications equipment used no closer to any part of the Podimetrics SmartMat, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended safety distance: $d = 1.2\sqrt{P}$ for 150 KHz to 80 MHz $d = 1.2\sqrt{P}$ for 80 MHz to 800 MHz $d = 2.3\sqrt{P}$ for 800 MHz to 2.5 GHz Where P as the maximum output power rating of the transmitter in watts [W] according to the transmitter manufacturer d as recommended separation distance in meters [m]. Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range. Interference may occur in the vicinity of equipment marked with the following symbol:
Electrostatic discharge (ESD) IEC 61000-4-2	±6kV Contact ±8kV Air	±6kV Contact ±8kV Air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transients / bursts IEC 61000-4-4	± 2 kV for power supply lines ± 1 kV for input / output lines	± 2 kV for power supply lines	Mains power quality should be that of a typical commercial or hospital environment.

Electromagnetic Immunity (continued):

The Podimetrics SmartMat is intended for use in the electromagnetic environment specified below. The customer or the user of the Podimetrics SmartMat should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Surge IEC 61000-4-5	± 1 kV line(s) to line(s) ± 2 kV line(s) to earth	± 1 kV line(s) to line(s) ± 2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	< 5% UT* (> 95% dip in the UT) for ½ cycle	< 5% UT* (> 95% dip in the UT) for ½ cycle	Mains power quality should be that of a typical commercial or hospital environment. If the user of the /operator of the Podimetrics SmartMat requires continued operation during power mains interruptions, it is recommended that the Podimetrics SmartMat be powered from an uninterruptible power supply or battery.
	40% UT (60% dip in the UT) for 5 cycles	40% UT (60% dip in the UT) for 5 cycles	
	70% UT (30% dip in the UT) for 25 cycles.	70% UT (30% dip in the UT) for 25 cycles.	
	< 5% UT (> 95% dip in the UT) for 5 s sec	< 5% UT (> 95% dip in the UT) for 5 s sec	
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

Note *: UT is the a.c. mains voltage prior to application of the test level.

Note 1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection of structures, objects, and people.

a) Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Podimetrics SmartMat is used exceeds the applicable compliance level above, the Podimetrics SmartMat should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the changing orientation or the location of the Podimetrics Mat.

b) Over the frequency range of 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

Electromagnetic Emissions:

The Podimetrics SmartMat is intended for use in the electromagnetic environment specified below. The customer or the user of the Podimetrics SmartMat should ensure that it is used in such an environment.

Emissions Test	Compliance	Electromagnetic Environment – Guidance
RF emissions CISPR 11	Group 1	The Podimetrics SmartMat uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The Podimetrics SmartMat uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause interference in nearby electronic equipment.
Harmonic emissions IEC 61000-3-2	Complies	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Complies	

⚠ **WARNING:** The use of accessories, transducers and/or cables other than those specified, with the exception of those sold by the manufacturer as replacement parts for internal components, may result in increased emissions or decreased immunity of the equipment or system.

⚠ **WARNING:** The equipment or system should not be used adjacent to or stacked with other equipment and that if adjacent or stacked use is necessary, the equipment or system should be observed to verify normal operation in the configuration in which it will be used.

RECOMMENDED SEPARATION DISTANCES

The following lists the recommended separation distances between portable and mobile RF communications equipment and the Podimetrics Mat

Recommended Separation Distances:

The Podimetrics SmartMat is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Podimetrics SmartMat can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Podimetrics SmartMat as recommended below, according to maximum output power of the communications equipment.

Rated maximum output power of transmitter [W]	Separation distance according to frequency of transmitter [m]		
	150 kHz to 80 MHz $d = 1.2\sqrt{P}$	80 MHz to 800 MHz $d = 1.2\sqrt{P}$	800 MHz to 2.5 GHz $d = 2.3\sqrt{P}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated by using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts [W] according to the transmitter manufacturer.

Note 1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

TECHNICAL INFORMATION

Operating Range:	59 to 104 °F (15 to 40 °C)
Storage and Transport:	-4 to 113 °F (-20 to 45 °C)
Operating Humidity:	15 to 93% RH, noncondensing
Operating Pressure:	700 hPa to 1060 hPa atmospheric pressure
Temperature Accuracy:	± 1 °F (± 0.6 °C)
Resolution:	0.2 °F (0.1 °C)
Normal Scan Time:	20 seconds
Spatial resolution of sensors:	0.56 inches (~14 mm) vertical and horizontal spacing
Device Dimensions:	22.9 x 16.1 x 1.2 inches
Device Weight:	7.5 lbs (3.4 kg)
Maximum User Weight:	375 lbs (170 kg)
Service life:	2 years of normal, daily use
Cellular Modem:	LTE radio, 750 MHz, 200 mW maximum output power
Battery:	Rechargeable lithium ion battery pack, 3.4 to 4.2 V, 1200 mAh, About 1 month of daily use.
Battery Charger:	Medical Power Supply; 100-240 V A/C, 50-60 Hz input; 5 V D/C max 1.2 A output, Mfg. P/N: GlobTek GTM41134-0606. Cable length: 60 inches
Product Certifications:	IEC 60601-1 3rd ed., IEC 60601-1-2 4th ed., IEC 60601-1-6 1st ed., IEC 60601-1-11 1st ed. NSFI High Traction Certified APMA Approved Device
Patents:	https://www.podimetrics.com/intellectual-property

TERMS OF USE AND PRIVACY POLICY
FOR PATIENTS USING THE PODIMETRICS SMARTMAT

Last Updated May, 2024

Terms of Use and Privacy Policy Summary:

If you use the SmartMat device, the services, and related materials, you are agreeing to the Terms of Use and Privacy Policy following this summary:

- The SmartMat measures the temperature of the soles of your feet when used properly with bare feet and transmits your temperature data to Podimetrics to enable communication with your healthcare provider regarding your footcare.
- The SmartMat does not replace physical examination by you or your healthcare provider, independently diagnose or guarantee prediction of foot ulcers or other conditions, replace regular self-examinations, or represent your internal body temperature.
- By using the SmartMat device, the services, and related materials, you agree to respect the intellectual property and legal rights of Podimetrics.
- We make no guarantees that the SmartMat, services and related materials will deliver any specific health outcome. We make no guarantees relating to others including your healthcare providers and healthcare plans.
- We will use arbitration to resolve any disputes you have with us related to your use of the SmartMat, Services or Related Materials on an individual basis.
- We will collect, use, and share your personal and health data only to operate the SmartMat device, services, and related materials as discussed in the Privacy Policy. Podimetrics may contact you and share your information with your healthcare provider, but we will not sell your health information.
- Podimetrics is regularly audited for compliance to data security and privacy standards.

TERMS OF USE FOR PATIENTS

Please read these terms of use (the "**Terms of Use**") carefully. **We have included a summary before this section to help explain the legal jargon and emphasize key sections. These annotations are for convenience only and have no legal or contractual effect.** The Terms of Use include disclaimers and limitations of liability, a class action waiver, and a waiver of jury trials. The Terms of Use also require binding arbitration on an individual basis to resolve disputes.

The Podimetrics SmartMat provides information indicating when a patient and healthcare provider should communicate for further evaluation and treatment regarding any persistent localized inflammation observed on a patient's feet.

The SmartMat is an in-home, daily-use floor mat that measures the temperature of a patient's feet and wirelessly transmits the temperature data to Podimetrics Inc. (**"Podimetrics"** or **"we"** or **"us"**) for processing and storage in the Podimetrics Cloud. The SmartMat is intended to be used by a patient in conjunction with a healthcare professional and/or caretaker for periodic evaluation of the temperature over the soles of the feet for signs of inflammation. Podimetrics may also provide certain care management services in connection with your use of the SmartMat. Each SmartMat is to be used by only one person.

The Podimetrics SmartMat is indicated for daily use in the home or clinical environment by people of all ages who are at risk of inflammatory conditions or injuries to the foot. It is for prescription use only. Your healthcare professional has identified you as someone who may benefit from use of the SmartMat. The SmartMat, and our Podimetrics Cloud and related services (the **"Services"**) and any additional websites and/or tools (individually and collectively, **"Related Materials"**), and your use thereof, are subject to these Terms of Use.

The SmartMat does not work for all patients and the efficacy of the SmartMat may vary. Due to the nature of cellular communications, the SmartMat may not be able to transmit data in all areas or at all times. Podimetrics is not a healthcare provider and the SmartMat, Services and Related Materials do not provide medical advice. Rather, the SmartMat, Services and Related Materials are a tool that your healthcare providers may use, in their professional

judgment, to inform their professional decision making. The SmartMat, Services, and Related Materials are not a replacement for a physical examination by a trained healthcare provider and should not be used independently to diagnose foot ulcers, inflammatory foot diseases, or other diseases or conditions. You should continue doing regular self-examinations. The measurement of plantar foot temperature is not a representative of your internal body temperature and it should not be used to evaluate a fever or your overall health. The quality or accuracy of a scan may be affected, for example, if you move your feet during a scan or if you are wearing socks.

The SmartMat, Services, and Related Materials are not, and do not provide, medical advice. You should not solely rely on the SmartMat, Services or Related Materials for the diagnosis or treatment of any health problem or disease. You should consult a healthcare professional or another qualified healthcare provider on a regular and appropriate basis.

IF YOU REQUIRE URGENT CARE, YOU SHOULD CONTACT YOUR LOCAL EMERGENCY SERVICES IMMEDIATELY.

By accessing or using the SmartMat, Services, or Related Materials, clicking on the "I agree" (or a similar) button, in connection with any Related Materials, or signing a document acknowledging and agreeing to these Terms of Use and returning the same to your healthcare provider or Podimetrics, you represent that (1) you have read, understand, and agree to be bound by the Terms of Use, (2) you are of legal age to form a binding contract with Podimetrics, and (3) you have the authority to enter into these Terms of Use with us personally. The term "you" refers to the individual who is provided the SmartMat or registered or authorized to use the SmartMat or Related Materials. **If you do not agree to be bound by the Terms of Use, you may not access or use the SmartMat, Services, or Related Materials and should return the SmartMat to Podimetrics or the healthcare provider who provided it to you.**

Please note that the terms are subject to change by Podimetrics in its sole discretion at any time. When changes are made,

Podimetrics will make a new copy of the Terms of Use available at our Website, https://podimetrics.com/terms-of-use, and/or may send you a hard copy of the revised Terms of Use to the address where the SmartMat is registered with us. We will also update the "Last Updated" date at the top of the Terms of Use. Any changes to the Terms of Use will be effective as of the effective date of the revised Terms of Use. If you do not agree to any change(s) after receiving a notice of such change(s), you shall stop using the SmartMat and Related Materials. If the SmartMat was made available to you on a loaner or temporary basis, you must immediately return the SmartMat to Podimetrics or the healthcare provider who provided it to you. Your continued use of the SmartMat and Related Materials constitutes your acceptance of such change(s). Please regularly check the website to view the then -current terms.

1. Use of SmartMat; Fees

1.1 General

You must use the SmartMat in accordance with these Terms of Use and the documentation we provide accompanying the SmartMat. You may not abuse or misuse the SmartMat or share it with another individual. You must return the SmartMat (ordinary wear and tear excepted) as instructed if you did not purchase it. The SmartMat may not work in all areas (e.g., where there is not wireless connectivity) or for all individuals. Consult with your healthcare provider regularly to confirm whether the SmartMat is transmitting appropriate data and for physical examinations. You may be granted use of the SmartMat, Services, and Related Materials through a Podimetrics customer ("Customer Patient") or directly through Podimetrics ("Self-Pay Patient").

1.2 Training and Support

We may offer you and/or your caregiver training with respect to your use of the SmartMat (and any updates, as applicable) over the telephone. In the event you experience any technical issues with the SmartMat, please contact Podimetrics for assistance.

1.3 Monitoring Services

We may contact you periodically at the phone number you provide us upon activation regarding your use of the SmartMat or the Services, including when we notice trends relating to your use (or non-use) of the SmartMat; to schedule in-home check-ins or follow-up appointments; and to communicate instructions from your healthcare provider.

1.4 Fees

Podimetrics charges certain fees for use of the SmartMat, Services, and Related Materials ("Podimetrics Fees"). Podimetrics Fees for Customer Patients are established between Podimetrics and the applicable customer. Podimetrics Fees for Self-Pay Patients are provided upon request and in advance of a Self-Pay Patient's enrollment with Podimetrics to receive the SmartMat, Services, and Related Materials. The Podimetrics Fees do not cover your interactions with your healthcare provider who prescribes the SmartMat for you and any other health care professionals you use outside of the Services.

2. Health Data

The SmartMat may transmit certain data relating to you and your feet to you and/or your healthcare provider and healthcare plan, and Podimetrics may be provided other data by you, your healthcare provider, and/or your healthcare plan, solely as permitted by applicable laws and regulations, including the Health Insurance Portability and Accountability Act of 1996 (HIPAA).

The privacy and security of such data will be protected by Podimetrics, and such data will be subject to the terms of our Privacy Policy available at https://podimetrics.com/privacy-policy. We will store your data transmitted to us by the SmartMat in the Podimetrics Cloud and use it to display your information to your healthcare provider. We may send or otherwise communicate that data to your healthcare provider when it indicates that you may need further evaluation and treatment, or otherwise to your healthcare plan if they are serving as or facilitating for your care management team. We may also share data with your caregiver if you consent to such sharing with your legal representative upon our verification of their authority to communicate on your behalf.

In some cases, we may use generative artificial intelligence services in connection with your use of the SmartMat, Services, and Related Materials. We ensure that appropriate agreements are in place with such services before making any of your data available to them.

In addition, we may analyze, aggregate, and/or de-identify that data to the extent permitted by applicable laws and regulations and applicable contracts to improve the SmartMat and Related Materials and/or develop and commercialize new products and services with de-identified data. You acknowledge and agree that Podimetrics exclusively owns such de-identified data and any improvements or new products or services arising therefrom.

We may also share your data with your healthcare provider and/or healthcare plan and as otherwise permitted under our Privacy Policy, subject to applicable laws and regulations.

3. Related Materials

3.1 General

We may make available Related Materials, such as websites, tools, information or other materials in connection with the SmartMat. Related Materials are protected by copyright and other laws throughout the world. Unless otherwise specified by Podimetrics in a separate license, your right to use any of the Related Materials is subject to these Terms of Use.

3.2 License

Subject to your compliance with the Terms of Use, Podimetrics grants you a limited non-exclusive, non-transferable, non-sublicensable, revocable license to access and use Related Materials for your personal use relating to your SmartMat. Some of the software in our Related Materials may be offered under an open source license that we make available to you. There may be provisions in the open source license that expressly override some of the Terms of Use, and you agree to be bound by the terms of such open source license.

3.3 Updates

You understand that Related Materials are evolving and may not be available. As a result, Podimetrics may require you to accept updates to Related Materials that you have installed. You acknowledge and agree that Podimetrics may update Related Materials with or without notifying you. You may need to update third-party software from time to time in order to access or use the Related Materials.

4. Certain Restrictions

The rights granted to you are subject to the following restrictions: (a) you shall not license, sell, rent, lease, transfer, assign, reproduce, distribute, host or otherwise commercially exploit the SmartMat or Related Materials or any portion thereof, (b) you shall not modify, translate, adapt, merge, make derivative works of, disassemble, decompile, reverse compile or reverse engineer any part of the SmartMat or Related Materials except to the extent the foregoing restrictions are expressly prohibited by applicable law; (c) you shall not use any means, including but not limited to script or programming, to scrape or mine the data or other content

associated with the SmartMat or Related Materials; (d) you shall not use the SmartMat or Related Materials in order to build a similar or competitive SmartMat, portal, application, or other product or service; (e) except as expressly stated herein, no part of the Related Materials may be copied, reproduced, distributed, republished, downloaded, displayed, posted or transmitted in any form or by any means; and (f) you shall not remove or destroy any copyright notices or other proprietary markings contained on or in the SmartMat or Related Materials. Any future release, update or other addition to the SmartMat or Related Materials shall be subject to the Terms. Podimetrics and its licensors, suppliers and service providers reserve all rights not granted in these Terms of Use.

5. Ownership

5.1 Podimetrics Intellectual Property.
You agree that Podimetrics and its suppliers own all rights, title and interest in and to the SmartMat, Services, and Related Materials and all intellectual property rights related to the SmartMat, Services and Related Materials. Physical devices may be owned by your healthcare provider, healthcare plan or Podimetrics and will be returned to the owner as requested.

5.2 Trademarks.
Podimetrics-related graphics, logos, service marks and trade names used on or in connection with the SmartMat or Related Materials are owned by Podimetrics and may not be used without permission. Other trademarks, service marks and trade names are the property of their respective owners.

5.3 Feedback.
You agree that submission of any ideas, suggestions, documents, and/or proposals to Podimetrics through its suggestion, feedback, wiki, forum or similar pages (**"Feedback"**) is at your own risk and that Podimetrics has no obligations (including without limitation obligations of confidentiality) with respect to such Feedback. You represent and warrant that you have all rights necessary to submit the Feedback. You hereby grant to Podimetrics a fully paid, royalty-free, perpetual, irrevocable, worldwide, non-exclusive, and fully sublicensable right and license to use, reproduce, perform, display, distribute, adapt, modify, re-format, create derivative works of, and otherwise commercially or non-commercially exploit in any manner, any and all Feedback, and to sublicense the foregoing rights.

6. Indemnification

You agree to indemnify and hold Podimetrics, its affiliates, officers, employees, agents, partners, and licensors (collectively the **"Podimetrics Parties"**) harmless from any losses, costs, liabilities and expenses (including reasonable attorneys' fees) relating to or arising out of: (a) your use of, or inability to use, the SmartMat or Related Materials; (b) your violation of the Terms of Use; or (c) your violation of any applicable laws, rules or regulations. Podimetrics reserves the right, at its own cost, to assume the exclusive defense and control of any matter otherwise subject to indemnification by you, in which event you will fully cooperate with Podimetrics in asserting any available defenses. You agree that the provisions in this section will survive any termination.

7. Disclaimer of Warranties

7.1 AS IS

YOU EXPRESSLY UNDERSTAND AND AGREE THAT TO THE EXTENT PERMITTED BY APPLICABLE LAW, YOUR USE OF THE SMARTMAT AND RELATED MATERIALS IS AT YOUR SOLE RISK, AND THE SMARTMAT AND RELATED MATERIALS ARE PROVIDED ON AN "AS IS" AND "AS AVAILABLE" BASIS, WITH ALL FAULTS. THE PODIMETRICS PARTIES EXPRESSLY DISCLAIM ALL WARRANTIES, REPRESENTATIONS, AND CONDITIONS OF ANY KIND, WHETHER EXPRESS OR IMPLIED, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OR CONDITIONS OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE AND NONINFRINGEMENT.

PODIMETRICS MAKES NO WARRANTY, REPRESENTATION OR CONDITION THAT: (1) THE SMARTMAT OR RELATED MATERIALS WILL BE APPROPRIATE FOR YOU OR MEET YOUR REQUIREMENTS; (2) YOUR USE OF THE SMARTMAT OR RELATED MATERIALS WILL BE UNINTERRUPTED, TIMELY, SECURE OR ERROR-FREE; (3) THE RESULTS, INCLUDING ANY ADVICE, COMMUNICATION, OR SUPPORT THAT MAY BE OBTAINED FROM OR IN CONNECTION WITH USE OF THE SMARTMAT OR RELATED MATERIALS WILL BE ACCURATE OR RELIABLE; OR (4) ANY TECHNICAL OR OTHER ERRORS WILL BE CORRECTED.

The SmartMat is not a replacement of a physical examination by a trained healthcare provider and should not be used independently to diagnose foot ulcers or other diseases or conditions.

PODIMETRICS DOES NOT GUARANTEE THE EFFICACY OF THE SMARTMAT OR RELATED MATERIALS OR ANY INFORMATION PROVIDED THROUGH SUCH SMARTMAT OR RELATED MATERIALS. NO RESULTS OF ANY KIND ARE GUARANTEED. NO ADVICE OR INFORMATION, WHETHER ORAL OR WRITTEN, OBTAINED FROM PODIMETRICS OR ANY DISTRIBUTOR OR THROUGH THE SMARTMAT OR RELATED MATERIALS WILL CREATE ANY WARRANTY NOT EXPRESSLY MADE HEREIN.

7.2 No Liability for Conduct of Third Parties

You acknowledge and agree that the Podimetrics parties are not liable, and you agree not to seek to hold the Podimetrics parties liable, for the conduct of third parties, including healthcare providers, healthcare plans, or operators of external sites, and that the risk of harm or injury from such third parties rests entirely with you.

8. Limitation of Liability; Release

8.1 Disclaimer of Certain Damages.

YOU UNDERSTAND AND AGREE THAT IN NO EVENT SHALL THE PODIMETRICS PARTIES BE LIABLE FOR ANY INDIRECT, INCIDENTAL, SPECIAL, EXEMPLARY, OR CONSEQUENTIAL DAMAGES OR FOR ANY DAMAGES RESULTING FROM LOSS OF USE, DATA, OR PROFITS, ARISING OUT OF OR IN CONNECTION WITH THE SMARTMAT OR RELATED MATERIALS, WHETHER OR NOT THE PODIMETRICS PARTIES HAVE BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES, OR FOR ANY DAMAGES FOR PERSONAL OR BODILY INJURY OR EMOTIONAL DISTRESS ARISING OUT OF OR IN CONNECTION WITH THE SMARTMAT OR RELATED MATERIALS, WHETHER BASED ON WARRANTY, COPYRIGHT, CONTRACT, TORT (INCLUDING NEGLIGENCE), PRODUCT LIABILITY OR ANY OTHER LEGAL THEORY.

8.2 Cap on Liability

UNDER NO CIRCUMSTANCES WILL THE PODIMETRICS PARTIES BE LIABLE TO YOU FOR AN AMOUNT TO EXCEED ONE HUNDRED DOLLARS ($100) OR THE AMOUNTS YOU PAID PODIMETRICS FOR THE SMARTMAT AND RELATED MATERIALS, IF ANY.

8.3 Release

You hereby release, waive, relinquish and forever discharge the

Podimetrics Parties from every past, present and future claim, demand and right of action of every kind and nature, known or unknown, related to the care your healthcare provider provides you or fails to provide you or the failure of the SmartMat to identify any issue. If you are a California resident, you hereby waive California Civil Code Section 1542, which states, "A general release does not extend to claims which the creditor does not know or suspect to exist in his or her favor at the time of executing the release, which, if known by him or her must have materially affected his or her settlement with the debtor."

9. Term and Termination

9.1 Term.

These Terms of Use commence on first use of the SmartMat or Related Materials and remain in full force and effect while you are in possession of the SmartMat and Related Materials, unless terminated earlier in accordance with the Terms of Use.

9.2 Termination of Services by Podimetrics.

Podimetrics has the right to, immediately and without notice, suspend or terminate the Terms of Use in connection with the SmartMat and/or applicable Related Materials if: (i) you have materially breached any provision of the Terms of Use; (ii) Podimetrics is required to do so by law (e.g., where the provision of SmartMat becomes unlawful), (iii) your healthcare plan discontinues its contract with or benefits through Podimetrics, or (iv) if your healthcare provider requests termination of the Podimetrics services. You agree that all such terminations for cause shall be made in Podimetrics' sole discretion and that Podimetrics shall not be liable to you or any third-party for any termination.

9.3 Termination by You.

If you want to terminate, you may do so by ceasing use of the SmartMat and Related Materials, and to the extent the SmartMat was loaned to you, returning such SmartMat to the appropriate party.

9.4 Effect of Termination

Termination may result in deletion of your passwords and all of your data from our live databases. Your data already in our possession or control may continue to be available to your healthcare provider consistent with applicable law. Upon termination, your rights will automatically terminate. All provisions of the Terms of Use which

by their nature should survive, shall survive, including without limitation, ownership provisions, warranty disclaimers, and limitations of liability.

10. International Users

The SmartMat and Related Materials are intended for use in the United States of America only. Data is controlled and stored by Podimetrics and its service providers from facilities in the United States of America. Podimetrics makes no representations that Mats or Related Materials are appropriate or available for use in other locations. Those who access or use the SmartMat or Related Materials from other jurisdictions do so at their own volition, are responsible for compliance with local law, and hereby grant Podimetrics consent to transfer such data to the United States.

11. Arbitration

11.1 Applicability of Arbitration Agreement.

Except as expressly provided herein, all claims and disputes (excluding claims for emergency injunctive relief as set forth below) in connection with the Terms of Use or the SmartMat or Related Materials provided by Podimetrics that cannot be resolved informally or in small claims court shall be resolved exclusively by binding arbitration on an individual basis under the terms of this arbitration provision ("**Arbitration Agreement**").

Unless otherwise agreed to, all arbitration proceedings shall be held in English. This Arbitration Agreement applies to you and Podimetrics, and to any subsidiaries, affiliates, agents, employees, predecessors in interest, heirs, successors, and assigns, as well as all authorized or unauthorized users or beneficiaries of the Mats or Related Materials.

11.2 Arbitration Rules.

Arbitration shall be initiated through the American Arbitration Association ("**AAA**"), an established alternative dispute resolution provider ("**ADR Provider**") that offers arbitration as set forth in this section. If AAA is not available to arbitrate, the parties shall agree to select an alternative ADR Provider. The rules of the ADR Provider shall govern all aspects of the arbitration, including but not limited to the method of initiating and/or demanding arbitration, except to the extent such rules are in conflict with the Terms of Use.

The AAA Consumer Arbitration Rules governing the arbitration are available online at www.adr.org or by calling the AAA at 1-800-778 -7879.

11.3 Authority of Arbitrator

If arbitration is initiated, the arbitrator will decide the rights and liabilities, if any, of you and Podimetrics, and the dispute will not be consolidated with any other matters or joined with any other cases or parties. The arbitrator shall have the authority to grant motions dispositive of all or part of any claim. The arbitrator shall have the authority to award monetary damages, and to grant any non-monetary remedy or relief available to an individual under applicable law, the AAA Rules, and the Terms.

The arbitrator shall issue a written award and statement of decision describing the essential findings and conclusions on which the award is based, including the calculation of any damages awarded. The arbitrator has the same authority to award relief on an individual basis that a judge in a court of law would have. The award of the arbitrator is final and binding upon you and Podimetrics.

11.4 Waiver of Jury Trial.

THE PARTIES HEREBY WAIVE THEIR CONSTITUTIONAL AND STATUTORY RIGHTS TO GO TO COURT (OTHER THAN A SMALL CLAIMS COURT) AND HAVE A TRIAL IN FRONT OF A JUDGE OR A JURY, instead electing that all claims and disputes shall be resolved by arbitration under this Arbitration Agreement. Arbitration procedures are typically more limited, more efficient and less costly than rules applicable in a court and are subject to very limited review by a court.

11.5 Waiver of Class or Consolidated Actions.

ALL CLAIMS AND DISPUTES WITHIN THE SCOPE OF THIS AGREEMENT MUST BE ARBITRATED ON AN INDIVIDUAL BASIS AND NOT ON A CLASS BASIS, AND CLAIMS OF MORE THAN ONE USER CANNOT BE ARBITRATED JOINTLY OR CONSOLIDATED WITH THOSE OF ANY OTHER. In the event that this subparagraph is deemed invalid or unenforceable neither you nor we are entitled to arbitration and instead claims and disputes shall be resolved in a court located in Boston, Massachusetts.

11.6 Small Claims Court

Notwithstanding the foregoing, either you or Podimetrics may bring an individual action in small claims court.

11.7 Emergency Injunctive Relief.

Notwithstanding the foregoing, either party may seek emergency injunctive relief before a state or federal court in order to maintain the status quo pending arbitration. A request for interim measures shall not be deemed a waiver of any other rights or obligations under this Arbitration Agreement.

12. General Provisions

12.1 Electronic Communications.

To the maximum extent permitted by law, you consent to receive communications from Podimetrics in an electronic form.

12.2 Assignment.

The Terms of Use, and your rights and obligations hereunder, may not be assigned, subcontracted, delegated, or otherwise transferred by you without Podimetrics' prior written consent, and any attempted assignment, subcontract, delegation, or transfer in violation of the foregoing will be null and void.

12.3 Questions.

If you have any questions for Podimetrics regarding these Terms of Use, please contact Podimetrics by emailing us at info@podimetrics.com. We will do our best to address your concerns. If you feel that your question has been addressed incompletely, we invite you to let us know for further investigation.

12.4 Limitations Period.

You and Podimetrics agree that any cause of action arising out of or related to the Terms of Use, the SmartMat, or Related Materials must commence within (1) year after the cause of action accrues. Otherwise, such cause of action is permanently barred.

12.5 Governing Law.

The Terms and any action related thereto will be governed and interpreted by and under the laws of the Commonwealth of Massachusetts, without giving effect to any principles that provide for the application of the law of another jurisdiction. The United Nations Convention on Contracts for the International Sale of Goods does not apply to this Agreement.

12.6 Notice.

Where Podimetrics requires that you provide an e-mail address, you are responsible for providing Podimetrics with your most current e-mail address. In the event that the last e-mail address you provided to Podimetrics is not valid, or for any reason is not capable of delivering to you any notices required/ permitted by the Terms of Use, Podimetrics' dispatch of the e-mail containing such notice will nonetheless constitute effective notice. You may give notice to Podimetrics at the following address: 100 Dover Street, Somerville, MA 02144. Such notice shall be deemed given when received by Podimetrics by letter delivered by nationally recognized overnight delivery service or first class postage prepaid mail at the above address.

12.7 Waiver.

Any waiver or failure to enforce any provision of the Terms on one occasion will not be deemed a waiver of any other provision or of such provision on any other occasion.

12.8 Severability.

If any provision of the Terms of Use is, for any reason, held to be invalid or unenforceable, the other provisions of the Terms of Use will remain enforceable, and the invalid or unenforceable provision will be deemed modified so that it is valid and enforceable to the maximum extent permitted by law.

12.9 Export Control.

You may not use, export, import, or transfer the SmartMat or Related Materials except as authorized by U.S. law and any other applicable laws. In particular, but without limitation, the SmartMat and Related Materials may not be exported or re-exported (a) into any United States embargoed countries; or (b) to anyone on the U.S. Treasury Department's list of Specially Designated Nationals or the U.S. Department of Commerce's

Denied Persons List or Entity List. You represent and warrant that (i) you are not located in a country that is subject to a U.S. Government embargo, or that has been designated by the U.S. Government as a "terrorist supporting" country and (ii) you are not listed on any U.S. Government list of prohibited or restricted parties. You acknowledge and agree that products, services or technology provided by Podimetrics are subject to the export control laws and regulations of the United States. You shall comply with these laws and regulations and shall not, without prior U.S. government authorization, export, re-export, or transfer Podimetrics products, services or technology, either directly or indirectly, to any country in violation of such laws and regulations.

12.10 Consumer Complaints

In accordance with California Civil Code §1789.3, you may report complaints to the Complaint Assistance Unit of the Division of Consumer Services of the California Department of Consumer Affairs by contacting them in writing at 400 R Street, Sacramento, CA 95814, or by telephone at (800) 952-5210.

12.11 Entire Agreement.

The Terms are the final, complete and exclusive agreement of the parties with respect to the subject matter hereof and supersedes and merges all prior discussions between the parties with respect to such subject matter.

12.12 End User Wireless Service Agreement.

By using the SmartMat, Services and/or Related Materials, you expressly understand and agree that you have no contractual relationship whatsoever with the underlying wireless service provider or its affiliates or contractors and that you are not a third-party beneficiary of any agreement between Podimetrics and the underlying carrier. The user hereby waives any and all claims or demands therefor.

End Terms of Use

PRIVACY POLICY

Podimetrics is committed to protecting your privacy and the security of your personal data and information. Podimetrics, Inc. ("**Podimetrics**" or "**we**" or "**us**") has developed this privacy policy to explain our practices regarding the collection, use and disclosure of certain information in connection with use of our mats, devices, systems, services, websites, applications, portals and other related materials and technologies (collectively, our "**Products and/or Services**") and the security technologies and procedures we use to safeguard such information. This Privacy Policy is referenced in our Terms of Use and applies to our Products and/or Services. Capitalized terms used but not defined herein shall have the meaning set forth in the Terms of Use or other related documentation.

1. Questions; Contacting Podimetrics; Reporting Complaints.

If you have any questions or concerns or complaints about our Privacy Policy or our data collection or processing practices, please contact us at the following e-mail address: info@podimetrics.com.

2. A Note to Users Outside of the United States.

The Products and Services are intended for use in the United States of America only. If you are a non U.S. user, please do not submit any personal or other data or use the Products and/or Services.

3. Types of Data we Collect.

"Personal Data" means data that allows someone to identify or contact an individual, including, for example, name, address, telephone number, e-mail address, as well as any other non-public information that is associated with or linked to any of the foregoing data. Personal Data includes the information that is collected from use of our Products and/or Services, such as patient health related data pertaining to foot temperatures ("**Health Data**"). **"Anonymous Data"** means data that is not associated with or linked to Personal Data; Anonymous Data does not, by itself, permit the identification of individual persons. We collect and use Personal Data, Health Data and Anonymous Data, as described below.

a. General.

- We may collect Personal Data, such as first and last name, gender, phone number, e-mail and mailing addresses, and/or location.
- If you provide us feedback or contact us via e-mail, we will collect your name and e-mail address, as well as any other content included in your communications, in order to send you a reply.
- If you contact us via phone, we may collect your name and phone number in order to respond to your inquiry and to monitor and provide support relating to your use of our Products and Services.
- We also collect other types of Personal Data that you provide to us voluntarily, such as registration numbers, other requested information relating to support, and medical history information (such as history of foot ulcers, neuropathy, and amputation).
- If you are a healthcare provider, we may also collect information such as your professional title, company name, and password in order to enable access to certain functions, features, and data relating to your patients.

b. Health Data

- Our Products and Services will automatically collect Health Data, including foot temperature when using our Products and/or Services.
- Patients, healthcare providers, and healthcare plans may also provide us other Health Data in connection with the use of our Products and Services, including but not limited to information collected in the course of providing support or monitoring related to an individual's use of the Products and Services, such as photographs taken by healthcare providers during in-person training, follow-up, or support visits.

c. Other

Information Collected by our Websites and Portal. Our websites may collect information, including browser type, operating system, IP address (a number that is automatically assigned to a computer when a user uses the Internet, which may vary from session to session), domain name, and/or a date/time stamp for each visit. We may also gather certain information automatically and store it in log files. This information includes IP addresses, browser type, Internet service provider, referring/exit pages, operating system, date/time stamp, and clickstream data.

- We may also use cookies to collect information. **"Cookies"** are small pieces of information that a website sends to your computer's hard drive while you are viewing the website. We may use both session Cookies (which expire once a web browser is closed) and persistent Cookies (which stay on a computer until deleted). This type of information is collected to make certain functions and features more useful and to tailor the experience for you.
- **Information Collected from Healthcare Providers.** We may receive Personal Data relating to Patients from their healthcare providers or healthcare plans. We may add this information to the information we have already collected about a patient.

4. How We Use Personal Data and Health Data

a. General.

We may disclose a patient's Personal Data and/or Health Data to his or her healthcare provider(s) and/or healthcare plan(s), including without limitation, patient biometric data and the frequency of a patient's recorded use of the SmartMat or other applicable Product and/or Service.

We may use a patient's Personal Data in order to:

- provide the Products and Services to you;
- measure, monitor, evaluate, repair, and improve the efficacy of our Products and/or Services;
- send administrative e-mail or other notifications (including by phone), such as connectivity issues, security advisories, or support and maintenance advisories;
- facilitate home visits, including support, training visits, or follow-up visits;
- communicate instructions and other information as authorized by a healthcare provider to a Patient;
- facilitate calls and appointments between healthcare providers and Patients; and
- send newsletters, surveys, offers, and other promotional materials related to our Products and Services and/or for other marketing purposes of Podimetrics. If you do not want us to use your Personal Data in this way, please follow the "unsubscribe" instructions in any email communication from us.

b. Creation of Anonymous Data.

We may collect or create Anonymous Data records from Personal Data and Health Data by excluding information that makes the data personally identifiable, or we may de-identify or aggregate Personal Data and Health Data. We analyze these types of data so that we may enhance existing, or develop new, Products and/or Services, and we reserve the right to use these types of data for any purpose and to disclose such data to third parties, such as healthcare providers, healthcare plans, or vendors or business partners that help us support the Products and/or Services in our sole discretion, unless expressly prohibited by applicable laws or regulations.

5. How We Share Personal Data and Health Data

We may disclose Personal Data and Health Data as described below and as described elsewhere in this Privacy Policy. We do not sell Personal Data or Health Data for monetary or other valuable consideration.

a. **Disclosures to Healthcare Providers and Healthcare Plans.** Health Data that is collected from a Product or Service will be shared with that patient's healthcare provider, healthcare plan, and/or healthcare team for healthcare purposes, including communicating with the patient about the patient's use of the Products and/or Services and the results and analysis obtained in connection therewith.

b. **Disclosures to Caregivers or Legal Representatives.** We may share data with your caregiver if you consent to such sharing or with your legal representative upon our verification of their authority to communicate on your behalf.

c. **Disclosures to Vendors Working for Podimetrics.** We may share Personal Data and Health Data, as applicable, with service providers, including without limitation third-party vendors or business partners that help us provide the Products and/or Services to you. These include vendors that provide us data processing, hosting, disaster recovery, telecommunication, or other services, including marketing to help us connect with you, for example to educate you on the

benefits of the SmartMat, Services, and Related Materials. Podimetrics may use generative artificial intelligence, including Open AI, services in connection with your Personal Data and Health Data. These service providers are not permitted to use Personal Data or Patient Data other than to provide the services requested by Podimetrics. We will only share Personal Data or Patient Data with service providers to the extent reasonably necessary for them to provide the services requested by Podimetrics.

d. **Disclosures to Affiliates**. We may share Personal Data and Health Data with our parents, affiliates, subsidiaries, or other companies under a common control (collectively, "**Affiliates**"), in which case we will require our Affiliates to honor this Privacy Policy.

e. **Disclosures in the Event of Corporate Restructuring.** We may share Personal Data and Health Data in connection with or during negotiation of any merger, financing, acquisition or dissolution, transaction or proceeding involving sale, transfer, divestiture, or disclosure of all or a portion of our business or assets. In the event of an insolvency, bankruptcy, or receivership, Personal Data may also be transferred as a business asset. If another company acquires our company, business, or assets, that company will possess the Personal Data and Health Data collected by us and will assume the rights and obligations regarding Personal Data and Patient Data as described in this Privacy Policy and required by applicable laws and regulations.

f. **Other Disclosures**. Podimetrics may disclose Personal Data and Patient Data if it believes in good faith that such disclosure is necessary (a) in connection with any legal investigation; (b) to comply with relevant laws or to respond to subpoenas or warrants served on Podimetrics; (c) to protect or defend the rights or property of Podimetrics, its Affiliates, and/or its or their partners, customers, or users; and/or (d) to investigate or assist in preventing any violation or potential violation of the law, this Privacy Policy, or our Terms of Use.

6. Third Party Websites.

Our websites may contain links to third-party websites. When

you click on a link to any other website or location, you will leave our website and go to another site and another entity may collect Personal Data or Anonymous Data from you. We have no control over, do not review, and cannot be responsible for, these outside websites or their content. Please be aware that the terms of this Privacy Policy do not apply to these outside websites or content, or to any collection of your Personal Data after you click on links to such outside websites. We encourage you to read the privacy policies of every website you visit. The links to third-party websites or locations are for your convenience and do not signify our endorsement of such third parties or their products, content or websites.

7. Choices Regarding Information.

You have several choices regarding use of information in connection with the Products and Services:

a. **Email Communications.** We may periodically send free newsletters and e-mails that directly promote the use of our Products and/or Services. When you receive newsletters or promotional communications from us, you may indicate a preference to stop receiving further communications from us and you will have the opportunity to "opt-out" by following the unsubscribe instructions provided in the e-mail you receive or by contacting us directly (please see contact information above). Despite your indicated e-mail preferences, we may send you service-related communications, including notices of any updates to our Terms of Use or Privacy Policy.

b. **Cookies.** If you decide at any time that you no longer wish to accept cookies from our applicable Products and/or Services for any of the purposes described above, then you can instruct your browser, by changing its settings, to stop accepting cookies or to prompt you before accepting a cookie from the websites you visit. Consult your browser's technical information. If you do not accept cookies, however, you may not be able to use all portions, functions, or features of certain Products and/or Services. If you have any questions about how to disable or modify cookies, please let us know at the contact information provided above.

c. **Do Not Track.** Some internet browsers may be configured to send a "Do Not Track" signal to websites that you visit. We currently do not respond to "Do Not Track" or similar signals. To find out more about "Do Not Track," please visit

http://www.allaboutdnt.com.

8. Security of Personal Data and Patient Data.

Podimetrics is committed to protecting the security of Personal Data and Patient Data. We use a variety of industry-standard security technologies and procedures to help protect Personal Data and Patient Data from unauthorized access, use, or disclosure. Your data is stored, disclosed, and used in compliance Health Insurance Portability and Accountability Act of 1996 ("HIPAA"), as required. No method of transmission or method of electronic storage is 100% secure, however. Therefore, while Podimetrics uses reasonable efforts to protect Personal Data and Patient Data, Podimetrics cannot guarantee its absolute security.

9. A Note about Children.

We do not intentionally gather Personal Data or Patient Data from individuals who are under the age of 13. If a child under 13 submits Personal Data or Patient Data to Podimetrics and we learn that the Personal Data or Patient Data is the information of a child under 13, we will attempt to delete the information as soon as possible. If you believe that we might have any Personal Data or Patient Data from a child under 13, please contact us at info@podimetrics.com.

10. Changes to This Privacy Policy.

This Privacy Policy is subject to occasional revision, and if we make any material changes in the way we use your Personal Data or Patient Data, we will notify you, such as by prominently posting notice of the changes on our website. These changes will be effective on the effective date of the revised Privacy Policy. If you do not wish to permit changes in our use of your Personal Data or Patient Data, you must notify us that you wish to deactivate your account with us. Continued use of our Products and/or Services, following notice of such changes shall indicate your acknowledgement of such changes and agreement to be bound by such changes.

End Privacy Policy

Manual Del Usario

SmartMat™

Parte del Sistema de Monitoreo Remoto de Temperatura Podimetrics™

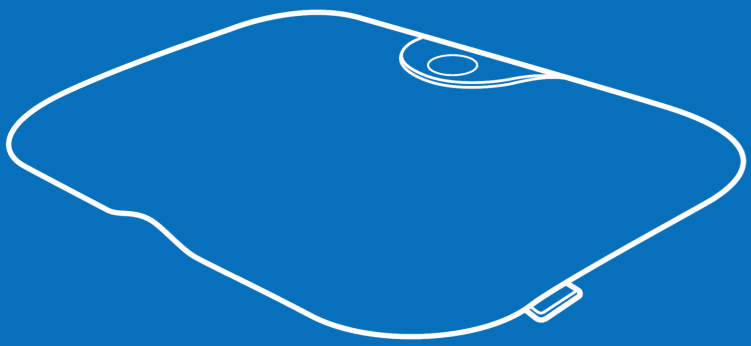

Construida en base a ciencia termométrica comprobada, la Podimetrics SmartMatTM registra escaneos térmicos diarios de alta resolución de sus pies y los transmite para que los evalúe su proveedor de atención médica.

podimetrics

INFORMACIÓN DE ASISTENCIA

Para ayuda técnica, por favor llame a Podimetrics, Inc.

Teléfono:	1-888-498-6489
Correo electrónico :	info@podimetrics.com
Correo :	Podimetrics, Inc. 100 Dover Street Somerville, MA 02144

Quejas relacionadas con la funcionalidad del equipo, desempeño o servicio pueden ser enviadas por correo o email.

ACERCA DE LA PODIMETRICS SMARTMAT ™

La Podimetrics SmartMat™ incluye componentes electrónicos sensibles para medir la temperatura en las plantas de los pies y transmitir esos datos de forma inalámbrica a un servidor remoto para evaluación. Los sensores de temperatura flexibles están ubicados directamente debajo de la cubierta y encima de una capa de espuma que se comprime cuando usted se para sobre esta. Cada escaneo térmico que se realiza con la SmartMat se transmite de forma inalámbrica a un servidor donde su proveedor de atención médica puede revisarlo para detectar signos de inflamación en sus pies.

INDICACIONES DE USO

El Sistema de Monitoreo Remoto de Temperatura™ Podimetrics (Sistema RTM™ Podimetrics, por sus siglas en Inglés) está destinada para ser utilizada por el paciente en colaboración de un profesional o asistente médico para la evaluación periódica de la temperatura en las plantas de los pies para buscar de señales de inflamación.

Esto proporcionará información que indicará cuando el paciente y el médico deben ponerse en contacto para realizar una evaluación y tratamiento posterior con respecto a cualquier inflamación localizada y persistente observada en los pies mediante el sistema de detección electrónico y visualización remota de los datos.

El sistema RTM™ Podimetrics debe ser utilizado bajo la orientación de un profesional médico como un complemento y no en reemplazo del autoexamen, cuidado y revisión periódica de los pies llevada a cabo por un profesional médico, éste no diagnostica ningún estado patológico específico.

Utilícese solamente bajo prescripción médica.

CONTRAINDICACIONES

Pacientes con una úlcera activa u otras lesiones que hayan roto la piel en las plantas de los pies no deben usar el Podimetrics SmartMat con el pie herido. Pacientes pueden continuar usando el Podimetrics SmartMat para monitorear el pie que no está herido.

DESEMPEÑO ESENCIAL

El desempeño esencial de la alfombra es realizar un escaneo completo y transmitir los datos de temperatura a un servidor remoto.

BENEFICIOS Y RIESGOS

Beneficios: Para los pacientes en riesgo de enfermedades inflamatorias del pie puede ser difícil evaluar las plantas de sus pies y detectar señales de inflamación relacionadas con una lesión. Los datos térmicos transmitidos de forma inalámbrica por la Podimetrics Mat™ pueden ser utilizados por usted y su médico para identificar señales de inflamación en los pies. Con esta información, su médico puede optar por iniciar un examen físico y tomar acciones para evitar complicaciones como úlceras en los pies, infecciones, gangrena y amputación.

Riesgos: La Podimetrics Mat™ no causa dolor o molestias cuando es utilizada. La capa superior ha sido probada para hacerla biocompatible con la piel. Si está dañada o es utilizada incorrectamente, pueden generarse lecturas de temperatura imprecisas que pueden afectar la evaluación médica de la inflamación.

⚠ ADVERTENCIAS

- **No utilice** la alfombra sin recibir previo entrenamiento de un médico profesional o un entrenador calificado.
- **No utilice** la alfombra si luce dañada o contaminada.
- **No utilice** la alfombra para más de una persona ya que puede resultar en contaminación cruzada o confusión de datos del paciente.
- Si presenta **irritación**, **enrojecimiento**, o **sarpullido** en las plantas de los pies, **deje de usarla** y contacte a su profesional médico inmediatamente.
- Si observa algún cambio en el comportamiento o funcionamiento de la alfombra, o daños causados por el transporte o uso, descontinue su uso y contacte a Podimetrics para recibir instrucciones.
- **No abra** o modifique este equipo en un intento para corregir un problema. En el interior no hay componentes que puedan ser manipulados por el usuario.

⚠ PRECAUCIONES

No coloque otros objetos o revestimientos sobre la alfombra cuando se esté utilizando. Los datos de la alfombra pueden resultar imprecisos si se utiliza con un revestimiento externo.

QUÉ PUEDE HACER CON SU ALFOMBRA

Viajando:
Siéntase libre de llevar su alfombra en la caja con usted y úsela en su destino. Especialmente cuando esté volando, apague la alfombra mientras que esté trasladándose. Si usted no planea llevar la alfombra con usted, llame a Podimetrics para notificar que usted no estará usando la alfombra.

Almacenamiento:
Guarde la alfombra apagada en su caja de envío en un lugar fresco, seco y alejado de la luz directa del sol. Los materiales pueden deteriorarse con el tiempo si son expuestos a la luz del sol o a temperaturas altas.

Retorno:
Contacte a Podimetrics para recibir instrucciones para regresar la alfombra usada. No deseche la alfombra en alguna instalación de residuo municipal ya que las partes electrónicas pueden dañar el medio ambiente.

SÍMBOLOS DE SEGURIDAD

No use el producto si el embalaje está dañado.

Lea cuidadosamente las instrucciones de uso.

IP 21

Este producto está calificado como IP21. Está protegido contra dedos insertados y goteo de agua.

La alfombra es una parte aplicada Tipo B.

Este producto contiene piezas electrónicas. No lo deseche en instalaciones de residuos municipales.

Rx only

Este producto es solamente para el uso bajo prescripción médica.

El dispositivo utiliza un transmisor de RF que produce radiación no ionizante.

QUÉ INCLUYE LA CAJA

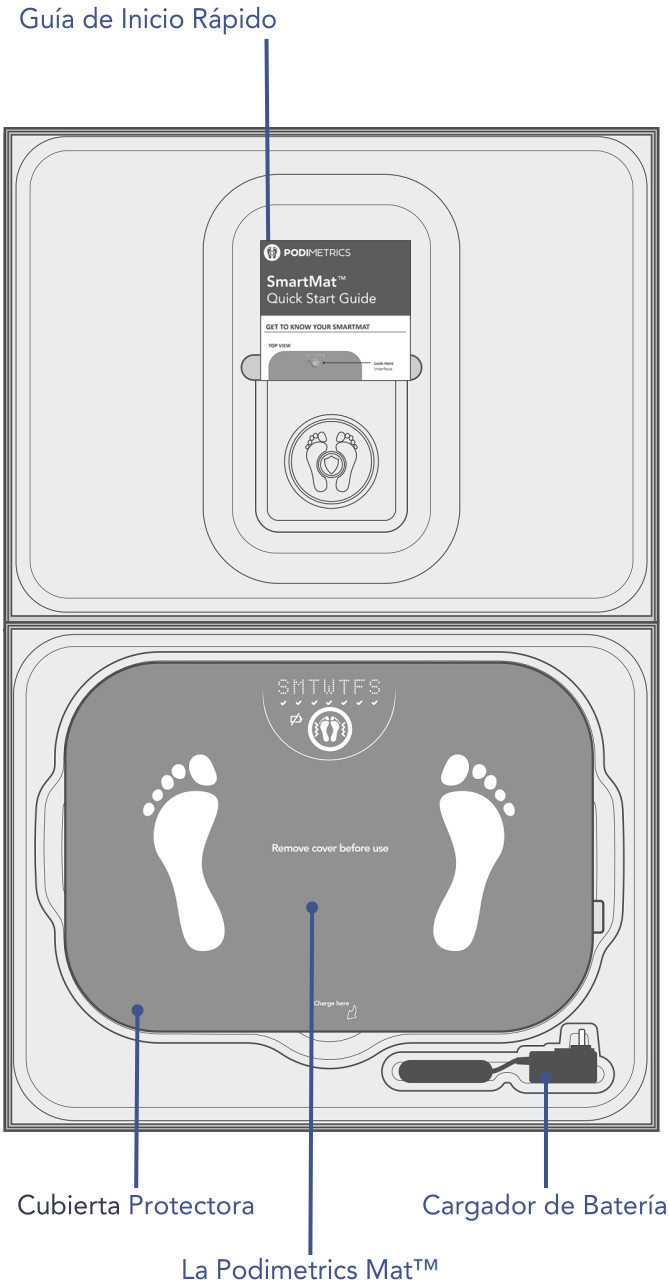

DESCRIPCIÓN DE LAS PIEZAS

PARTE SUPERIOR

LADO



PARTE INFERIOR

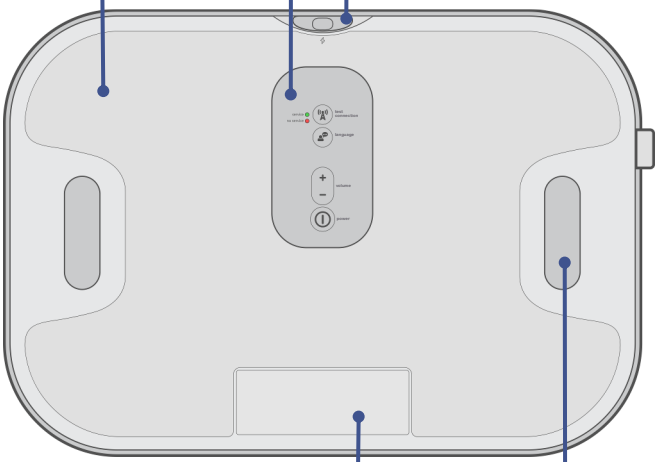

INSTRUCCIONES DE CONFIGURACIÓN

1. Pliegue hacia atrás la cobertura de plástico transparente y saque la alfombra de la caja: Pliegue hacia atrás la cobertura de plástico y con ambas manos saque la alfombra de la caja y colóquela sobre una mesa con los botones hacia arriba. No use la alfombra si luce dañada o contaminada.

> **NOTA: Conserve la caja** para guardar el cargador y las instrucciones, y para enviar la alfombra de regreso a Podimetrics despues de usarla.

2. Encienda la alfombra: Presione el botón de encendido (Power). Cuando escuche la campanilla de inicio, la alfombra está lista para su uso. **Nota: Mantenga la alfombra encendida en todo** momento para que ésta pueda enviar sus datos.

3. Ajuste el volumen: Hay cuatro ajustes de volumen, Apagado, Bajo, Medio, y Alto. Presione el botón para aumentar el volumen (+) o disminuir el volumen (-) hasta que el tono audible alcance el nivel deseado.

4. Ajuste el idioma: Presione el botón de idioma ("language") para cambiar el idioma de los mensajes. El último idioma que escuche será guardado para el futuro.

5. Revise el servicio celular: La alfombra se conecta automáticamente a una red celular, justo como un teléfono celular. Para asegurarse de que la alfombra pueda enviar sus datos, compruebe el servicio celular presionando el botón de comprobar servicio celular (check cellular service) y espere a que el indicador de luz de color se encienda. Si la luz roja ("no service") se enciende, mueva la alfombra hacia una ubicación diferente e intente de nuevo.

PANEL DE BOTONES
(EN LA PARTE INFERIOR DE LA ALFOMBRA)

COMPRUEBE EL SERVICIO CELULAR
(EN EL PANEL DE BOTONES)

6. Ubique la alfombra para su uso: Coloque la alfombra sobre una superficie plana donde no esté obstruida por otros objetos y donde usted pueda pararse cómodamente por al menos 20 segundos. El lado de color gris claro debe estar hacia arriba.

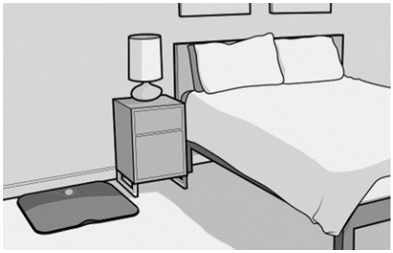

UBICACIÓN RECOMENDADA PARA LA ALFOMBRA

⚠ CUIDADO:

- **No coloque** la alfombra en un área de mucho tráfico como en un pasillo o una entrada
- **No coloque** la alfombra en un lugar donde pueda mojarse, como cerca de la ducha
- **No coloque** la alfombra bajo la luz directa del sol o cerca de fuentes de calor como ventanillas o aparatos de calefacción
- Coloque la alfombra en un lugar donde pueda minimizar el riesgo de manipulación por niños o mascotas
- Coloque la alfombra en una posición en la que usted pueda desenchufarla fácilmente antes de usarla.

LUZ DE RECORDATORIO DIARIO

Cada día, si usted no ha realizado el escaneo ese día a las 9:00AM la luz azul de recordatorio se iluminará. Usted siempre puede realizar un escaneo antes de que la luz de recordatorio se encienda.

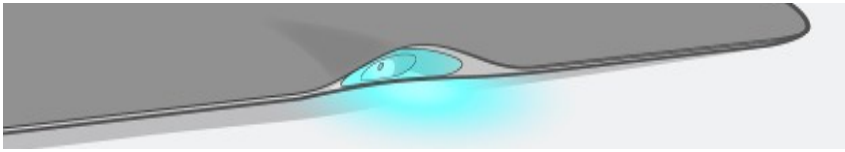

INSTRUCCIONES DE USO

NOTA: Para obtener los mejores resultados, siga este proceso cada mañana.

1. Realice un examen del pie diariamente:

Siga realizando su inspección diaria del pie, como ha sido indicado por su profesional médico, examinando sus pies en busca de señales de úlceras en desarrollo o heridas abiertas.

ADVERTENCIA: Si usted nota piel rota o una úlcera en desarrollo, detenga el uso de la alfombra y contacte a su profesional médico de inmediato.

2. Revise la alfombra:

Antes de usar, revise la alfombra en busca de humedad, daño o decoloración. Asegúrese de que la alfombra esté seca antes de usarla. Si está dañada, no use la alfombra y contacte a Podimetrics para obtener un reemplazo. Si está decolorada, trate de remover cualquier residuo. Si la decoloración no puede ser removida, contacte a Podimetrics para determinar si un reemplazo es necesario.

CUIDADO: No use la alfombra cuando haya agua o loción en sus pies.

3. Párese sobre la alfombra, descalzo:

Para comenzar un escaneo, párese sobre el lado gris claro de la alfombra con ambos pies completamente sobre la alfombra. La pantalla mostrará “QUEDESE QUIETO”. Una vez que usted esté parado relajado, el escaneo comenzará automáticamente. Si su doctor recomienda que usted continúe usando la alfombra con una herida vendada, párese sobre la alfombra sólo con el pie que no está vendado. Siempre siga las instrucciones de su doctor con respecto a calzado.

NOTA: No deje la alfombra enchufada. La alfombra no puede realizar un escaneo con batería baja o cuando está enchufada.

NOTA: Aunque el uso de pie es preferible, la alfombra también puede ser usada cuando usted está sentado mientras que la suficiente presión sea aplicada para completar un escaneo. No use la alfombra en una manera que usted sienta que pueda incrementar su riesgo de caída o tropiezo. Hable con su médico sobre si usar la alfombra de pie o sentado es más apropiado para usted.

4. Complete el escaneo:

Mantenga sus pies quietos por 20 segundos mientras el escaneo se completa. El círculo de progreso se llenará completamente y se volverá blanco cuando el escaneo sea completado. Se mostrará "ESCANEO GUARDADO!" y la alfombra emitirá una campanilla de nuevo. Usted ahora podrá retirarse de la alfombra.

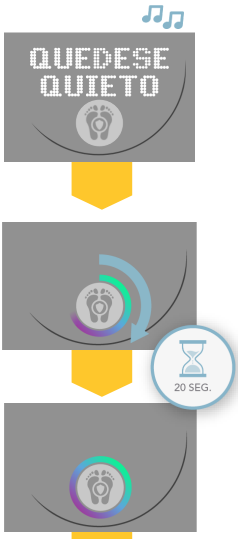

NOTA: Si usted mueve sus pies durante el escaneo, el icono de estabilidad se iluminará y una campanilla de error sonará, indicando que el escaneo se ha interrumpido. Párese quieto para que el escaneo se reinicie.

5. Revise los escaneos y la batería semanalmente:

La alfombra mostrará su calendario semanal de escaneos y confirmará el escaneo de hoy. Una marca de verificación ✔ significa que un escaneo ya fue realizado ese día. El porcentaje del nivel de batería es mostrado en la pantalla. Su escaneo será transmitido automáticamente y la alfombra entrará en modo inactivo. Mantenga la alfombra encendida para que su escaneo sea transmitido

NOTA: Usted puede chequear rápidamente sus escaneos recientes y el nivel de batería al presiona la parte superior de la alfombra.

TRANSMISIÓN DE DATOS Y NOTAS DE MONITOREO

Los datos se transmiten automáticamente: Si usted ha colocado la alfombra en un lugar con buena señal celular (vea la página 8 para instrucciones sobre cómo verificar la señal celular) la alfombra transmitirá automáticamente los datos a Podimetrics a través de la red celular. La cobertura celular puede no estar disponible en todas las regiones. Contacte a Podimetrics si tiene dificultad para encontrar un lugar con buena o decente señal. La información puede no ser transmitida fuera de los Estados Unidos.

Monitoreo de Podimetrics: Si Podimetrics no ha recibido un escaneo proveniente de su alfombra en algún tiempo, usted puede que reciba una llamada para asegurarnos de que todo esté bien con y su alfombra.

Revisión de escaneo: su proveedor de atención médica puede revisar los datos de su SmartMat periódicamente para detectar signos de inflamación. Los informes recibidos muestran imágenes térmicas de sus pies y le permiten a su proveedor de atención médica analizar áreas de temperatura elevada para cada escaneo que es transmitido. Consulte a su médico para obtener información sobre la evaluación del termograma.

LIMPIEZA

Limpieza: Una vez por mes o cuando sea necesario, limpie la superficie superior de la alfombra usando agua tibia y un paño limpio para remover cualquier sucio o residuo que pueda asentarse y afectar al sensor de lectura o hacerla resbaladiza. Deje que la alfombra se seque al aire antes de usarla. Si para usted es difícil limpiar mientras la alfombra está en el suelo, usted puede colocarla sobre una mesa.

⚠ **CUIDADO:** No limpie la alfombra con jabón ya que puede dejar un residuo resbaladizo. No sumerja la alfombra en agua.

CARGANDO LA BATERÍA

Cargando la batería: La luz de batería baja se encenderá cuando la batería sea muy baja como para realizar un escaneo. Para cargarla, coloque la alfombra hacia abajo sobre una mesa o mostrador cerca de un enchufe eléctrico. Conecte el cargador a un enchufe estándar de pared e inserte el extremo redondo en el puerto de carga. Cargar una batería vacía tarda alrededor de 4 horas. Mientras la alfombra está conectada, no podrá realizar escaneos.

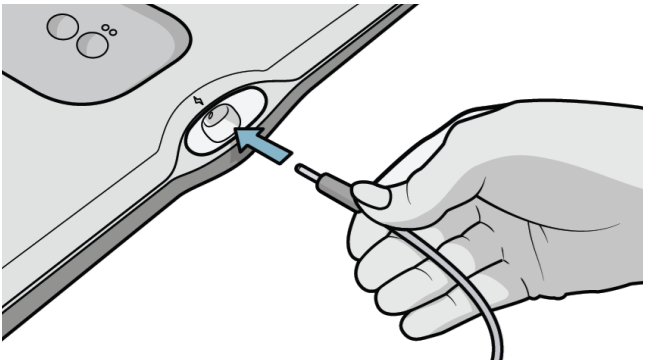

UBICACIÓN DEL CARGADOR
(EN EL LADO DE LA ALFOMBRA)



CARGANDO
(DESTELLO AMARILLO)

CARGA COMPLETA
(VERDE SÓLIDO)

NOTA: Desconecte la alfombra antes de realizar un escaneo de nuevo. Si usted se para sobre la alfombra mientras que está conectada, una campanilla de error sonará y "DESCONECTE" (UNPLUG) será mostrado en la pantalla.

⚠ CUIDADO:

- Use solo el cable del cargador provisto para cargar. Usar otros cables pueden dañar las piezas electrónicas internas.
- Mantenga el cable del cargador fuera del suelo y alejado de pasillos para evitar crear un peligro de caída.
- Mantenga el cable del cargador fuera del alcance de los niños. El cable del cargador puede ser un riesgo de estrangulación
- Su cargador puede que no funcione en otros países.

SOLUCIÓN DE PROBLEMAS

Si las instrucciones en esta tabla no resuelven el problema o si usted experimenta algún malfuncionamiento o lesión, por favor llame al servicio técnico de Podimetrics al 1-888-498-6489.

Problema	Significado	Acción
Se enciende la luz de "Batería baja"	La batería está baja.	Conecte el cargador para cargar la batería de la alfombra durante la noche.
Se enciende la luz de "Sin servicio"	La alfombra no tiene suficiente señal celular en esta ubicación.	Mueva la alfombra a un área con mejor cobertura de señal celular, como cerca de una ventana o en un piso superior.
Se enciende la luz de "Error de estabilidad"	Tal vez sus pies se movieron durante el escaneo.	Asegúrese de que ambos pies estén completamente dentro de la zona con sensores y quedese quieto hasta que se complete el escaneo.
El escaneo no inicia después de que usted se para sobre la alfombra.	La alfombra puede estar apagada. - o - La batería puede estar descargada	Si no hay ninguna luz encendida, intente presionar el botón de aumentar el volumen (+). Si la alfombra no emite ningún sonido, presione el botón de encendido para encender la alfombra. Si la alfombra aun no enciende, tal vez necesite cargar la batería.
La alfombra no emite ningún sonido.	Puede que el volumen no esté encendido.	Presione el botón de aumentar el volumen (+) en la parte inferior de la alfombra para encender el volumen.

INFORMACIÓN TÉCNICA

Rango Operacional:	59 to 104 °F (15 to 40 °C)
Almacenamiento y Transporte:	-4 to 113 °F (-20 to 45 °C)
Humedad Operacional:	15 to 93% RH, sin condensación
Presión Operacional:	700 hPa to 1060 hP presión atmosférica
Precisión de Temperatura:	± 1 °F (± 0.6 °C)
Resolución:	0.2 °F (0.1 °C)
Tiempo de Escaneo:	20 segundos
Resolución espacial de sensors:	0.56 pulgadas (~14 mm) espacio vertical y horizontal
Dimensiones del dispositivo:	22.9 x 16.1 x 1.2 pulgadas
Peso del dispositivo:	7.5 libras (3.4 kg)
Peso máximo del usuario:	375 libras (170 kg)
Vida de servicio:	2 años de uso normal diario
Módem Celular:	PMHS201U: LTE radio, 750 MHz, 200 mW máxima salida de poder
Batería:	Batería de litio recargable, 3.4 a 4.2 V, 1200 mAh, About 1 meses de uso diario.
Cargador de Batería:	Suministro de energía médica; 50-60 Hz entrada; 5 V D/C máximo 1.2 A salida, Mfg. P/N: Globtek GTM41134-0606. Longitud máxima del cable: 60 pulgadas.
Certificaciones del Producto:	IEC 60601-1 3ra ed., IEC 60601-1-2 4ra ed., IEC 60601-1-6 1ro ed., IEC 60601-1-11 1ro ed. NSFI Certificado de Alta Tracción Dispositivo Aprobado por APMA
Patentes:	https://podimetrics.com/intellectual-property

NOTES / NOTAS

Consejos para usar la SmartMat™

1. Utilice la SmartMat descalzo todos los días con los pies separados.
2. Si se siente inestable de pie, complete el escaneo mientras está sentado.
3. Mantenga la SmartMat encendida en todo momento.
4. Cargue su alfombra cuando la batería baje al 10%.
5. No pise el SmartMat con un pie con una herida abierta.
6. La luz azul de recordatorio parpadeará durante el día si usted aún no ha completado el escaneo ese día, pero usted puede completar su escaneo en cualquier momento.

1-888-498-6489

info@podimetrics.com

Tips for using your SmartMat™

1. Use the SmartMat barefoot every day with your feet spread apart.
2. If you feel unsteady on your feet, take your scan while sitting.
3. Keep the SmartMat turned on at all times.
4. Charge your SmartMat when the battery is down to 10%.
5. Do not step on the SmartMat with a foot with an open wound.
6. The blue reminder light will blink during the day if you haven't scanned yet that day, but you can take your scan at any time.

1-888-498-6489

info@podimetrics.com

podimetrics

100 Dover Street
Somerville, MA 02144
https://www.podimetrics.com

© 2024 Podimetrics, Inc. All rights reserved.

LBL-0029 rev H | Updated June, 2024